



# Confirm that the Color Sequence Matches

The black reference electrode is on this side.

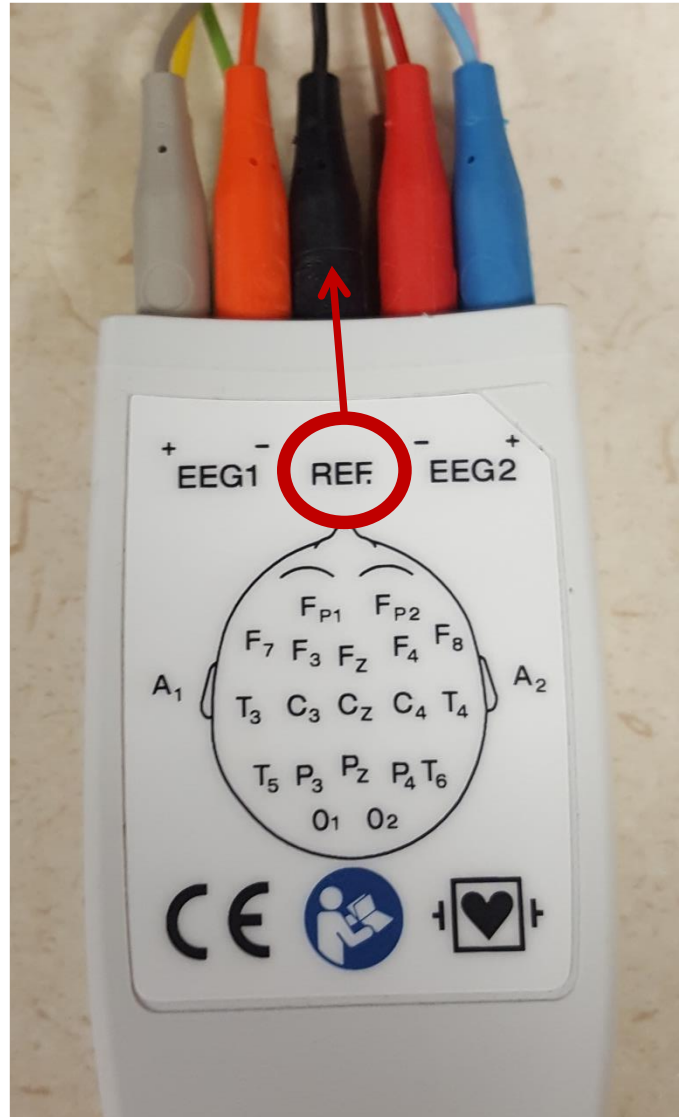

# Connect Electrode to Match Colors as Shown

Right: Even Numbers  
Left: Odd numbers

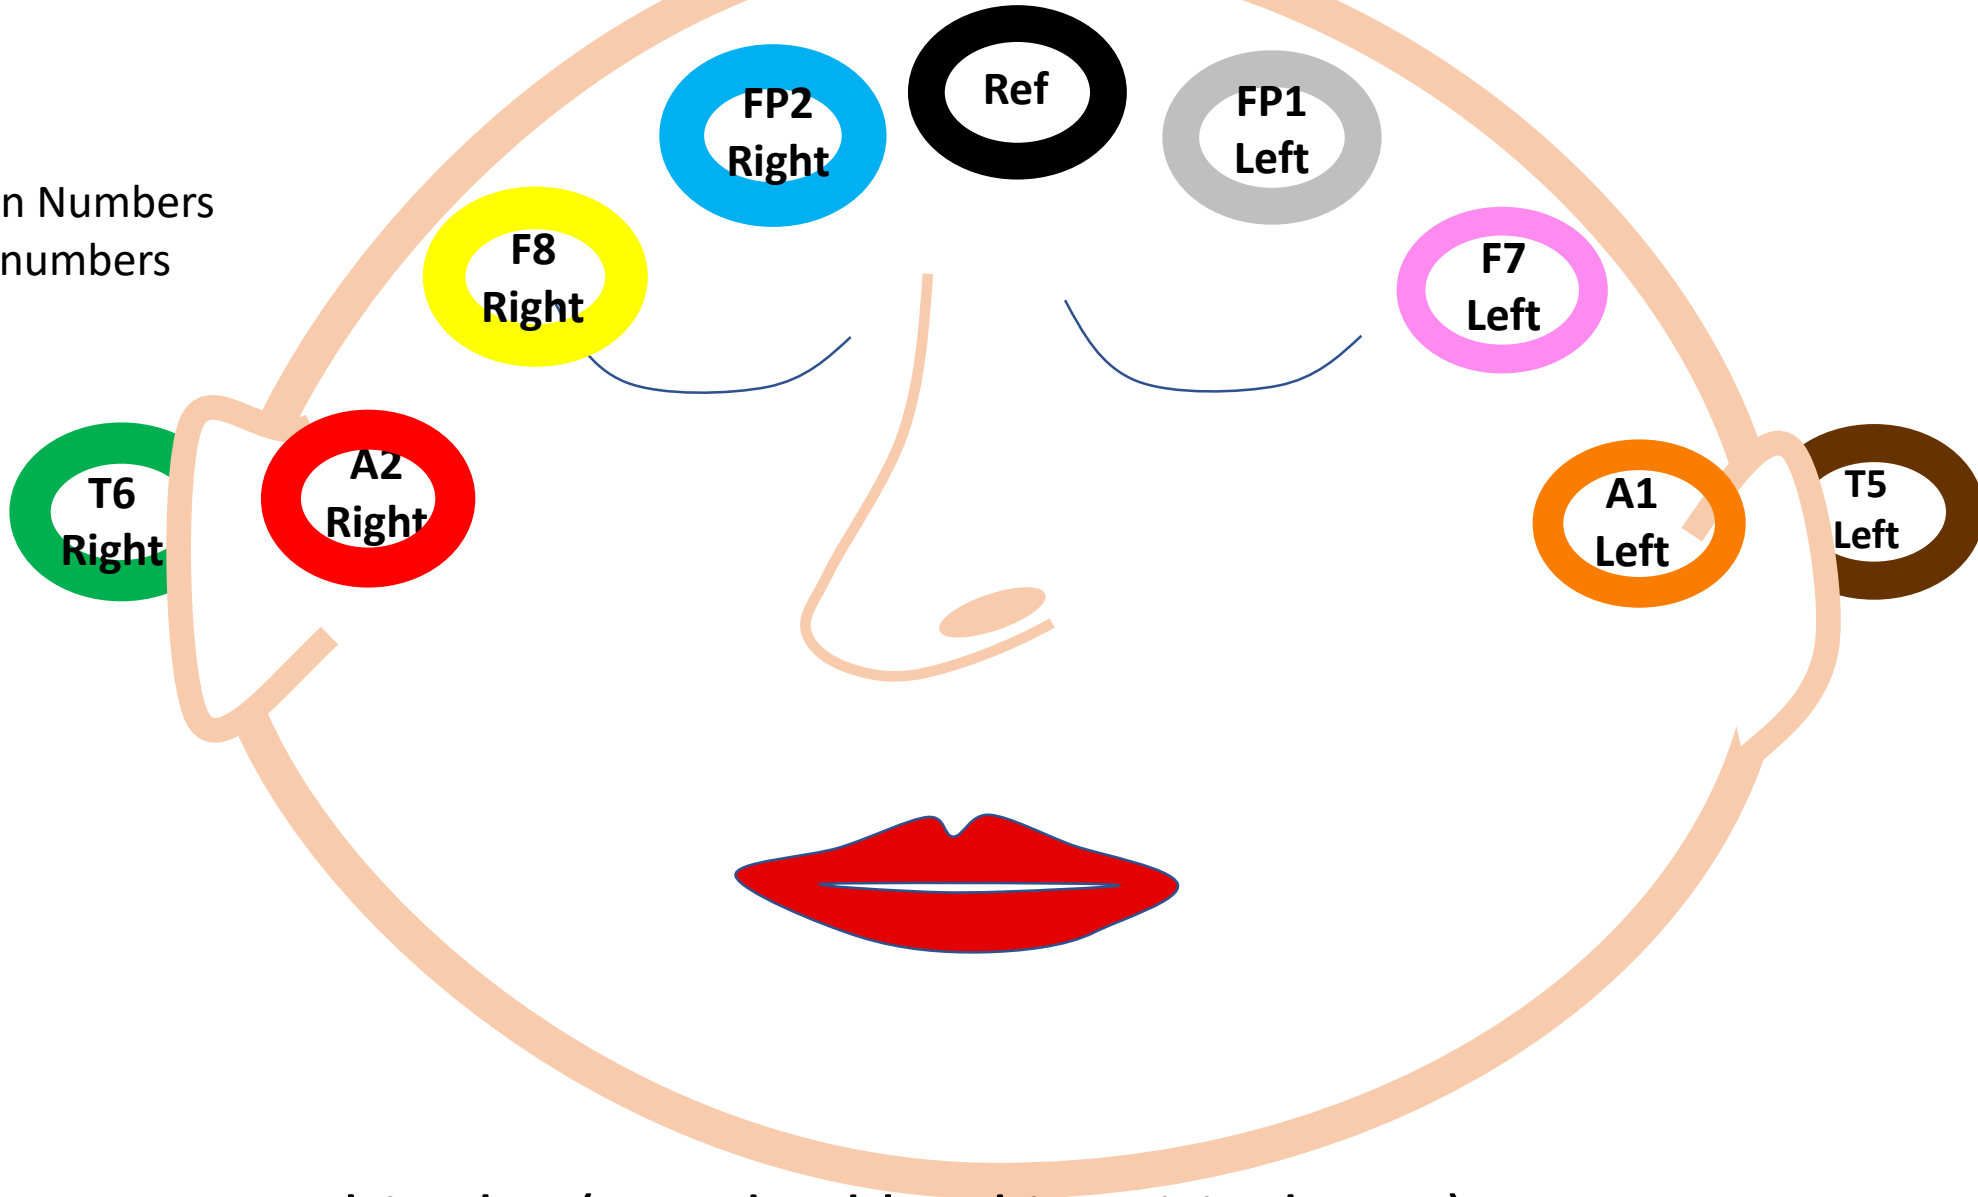

**Montage A:** Long bipolar (standard lead in critical care)

2020-08-11